







Wafer probe station having integrated guarding, Kelvin connection and shielding systems.

Patent number: EP0574149
Publication date: 1993-12-15
Inventor: SCHWINDT RANDY J (US); HARWOOD WARREN K (US); TERVO PAUL A (US); SMITH KENNETH R (US); WARNER RICHARD H (US); ANDREWS PETER D (US)
Applicant: CASCADE MICROTECH INC (US)
Classification:
- international: **G01R1/067; G01R31/28; H01L21/687; G01R1/067; G01R31/28; H01L21/67; (IPC1-7): H01L21/00**
- european: **G01R1/067B; G01R31/28G5; H01L21/687S**
Application number: EP19930303936 19930520
Priority number(s): US19920896853 19920611

Also published as:

 US5345170 (A1)
 JP6053293 (A)
 EP0574149 (B1)

Cited documents:

 EP0201205
 US4056777
 XP000095937

[Report a data error here](#)

Abstract of EP0574149

A probe station is equipped with an integrated guarding system which facilitates the use of the station for low-current measurements, as well as integrated Kelvin connections to eliminate voltage losses caused by line resistances. The station has a chuck assembly (20) which consists of at least three chuck assembly elements (80, 81, 83). A first element (80) supports the test device, while an underlying second element (81) acts as a guard to reduce leakage currents. These elements are electrically insulated from each other and from their underlying supporting structure, which is the third element (83). Ready-to-use, selectively detachable electrical connector assemblies (108, 110) provide for signal and guard connections to the first and second chuck assembly elements (80, 81) respectively, as well as providing Kelvin connections thereto. The capacitance between the respective chuck assembly elements (80, 81, 83) is extremely low due to the provision of air space as the primary electrical insulator. Unique electrical connectors (128, 130) for individually-positionable probes (30) provide both guarding and Kelvin connection capability together with separate EMI shielding movable in unison with each probe individually.

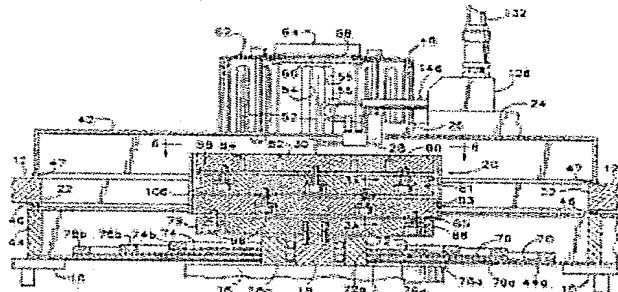


Fig. 3

Data supplied from the **esp@cenet** database - Worldwide



Europäisches Patentamt
European Patent Office
Office européen des brevets



Publication number: **0 574 149 A1**

(12)

EUROPEAN PATENT APPLICATION

(21) Application number: **93303936.4**

(51) Int. Cl.⁵: **H01L 21/00**

(22) Date of filing: **20.05.93**

(30) Priority: **11.06.92 US 896853**

(43) Date of publication of application:
15.12.93 Bulletin 93/50

(84) Designated Contracting States:
DE FR GB IT

(71) Applicant: **CASCADE MICROTECH, INC.**
14255 S.W. Brigadoon Ct.,
Suite C,
Beaverton Oregon 97005(US)

(72) Inventor: **Schwindt, Randy J.**
2940 S.E. Tacoma
Portland, Oregon 97202(US)
Inventor: **Harwood, Warren K.**
8505 N.E. 140th Avenue
Vancouver, Washington 98682(US)
Inventor: **Tervo, Paul A.**

3011 N.E. 157th Avenue
Vancouver, Washington 98682(US)

Inventor: **Smith, Kenneth R.**
7245 S.W. Ashdale

Portland, Oregon 97223(US)

Inventor: **Warner, Richard H.**
1834 S.E. Exeter Drive

Portland, Oregon 97202(US)

Inventor: **Andrews, Peter D.**
10575 S.W. Tigard Street, No. 38
Tigard, Oregon 97223(US)

(74) Representative: **Skerrett, John Norton Haigh**
et al
H.N. & W.S. SKERRETT
Charles House
148/9 Great Charles Street
Birmingham B3 3HT (GB)

(54) **Wafer probe station having integrated guarding, Kelvin connection and shielding systems.**

(57) A probe station is equipped with an integrated guarding system which facilitates the use of the station for low-current measurements, as well as integrated Kelvin connections to eliminate voltage losses caused by line resistances. The station has a chuck assembly (20) which consists of at least three chuck assembly elements (80, 81, 83). A first element (80) supports the test device, while an underlying second element (81) acts as a guard to reduce leakage currents. These elements are electrically insulated from each other and from their underlying supporting structure, which is the third element (83). Ready-to-use, selectively detachable electrical con-

nector assemblies (108, 110) provide for signal and guard connections to the first and second chuck assembly elements (80, 81) respectively, as well as providing Kelvin connections thereto. The capacitance between the respective chuck assembly elements (80, 81, 83) is extremely low due to the provision of air space as the primary electrical insulator. Unique electrical connectors (128, 130) for individually-positionable probes (30) provide both guarding and Kelvin connection capability together with separate EMI shielding movable in unison with each probe individually.

E 0 574 149 A1

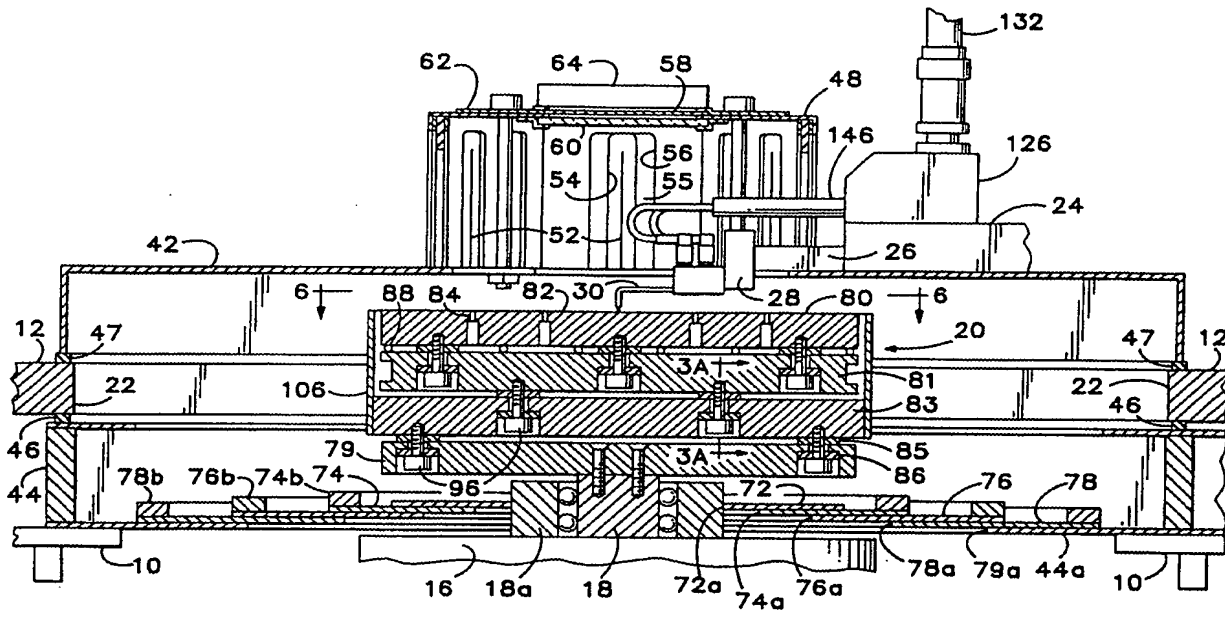


Fig. 3

Background of the Invention

The present invention is directed to probe stations adapted for making highly accurate low-current and low-voltage measurements of wafers and other electronic test devices. More particularly, the invention relates to such a probe station having a guarding system for preventing current leakage, a Kelvin connection system to eliminate voltage losses caused by line resistances, and an electromagnetic interference (EMI) shielding system.

The technique of guarding to minimize current leakage during low-current measurements, the use of Kelvin connections for low-voltage measurements, and the provision of EMI shielding are all well known and discussed extensively in the technical literature. See, for example, an article by William Knauer entitled "Fixturing for Low-Current/Low-Voltage Parametric Testing," appearing in *Evaluation Engineering*, November, 1990, pages 150-153. See also Hewlett-Packard, "Application Note 356-HP 4142B Modular DC Source/Monitor Practical Application," (1987) pages 1-4, and Hewlett-Packard, *H-P Model 4284A Precision LCR Meter, Operation Manual* (1991) pages 2-1, 6-9, and 6-15.

In guarding applications, a conductor surrounding or otherwise closely adjacent to a low-current line or circuit is maintained at the same potential as the line or circuit to reduce leakage currents therefrom, so that low-current measurements can be made accurately.

Kelvin connections compensate for voltage losses caused by line resistances which would otherwise cause errors in low-voltage measurements. This is accomplished by providing a source line and a measurement line (also referred to commonly as "force" and "sense" lines, respectively) to an interconnection point (the Kelvin connection) which is as close to the test device as possible. A high-impedance voltmeter is connected to this interconnection point through the measurement line to accurately detect the voltage without any significant flow of current or resultant voltage drop in the measurement line. This avoids the error which would otherwise occur if the voltmeter were to detect the voltage through the source line, due to the voltage drop that occurs in the source line.

Probe stations have previously been used for conducting tests with guarding, Kelvin connection, and EMI shielding techniques. However the custom set-up of such probe stations required for guarding and Kelvin connection procedures is time-consuming and, in some instances, limited as to effectiveness. For example, in an article by Yousuke Yamamoto, entitled "A Compact Self-Shielding Prober for Accurate Measurement of On-Wafer Electron Devices," appearing in *IEEE Transactions on*

Instrumentation and Measurement, Volume 38, No. 6, December, 1989, pages 1088-1093, a probe station is shown having a respective detachable triaxial connector mounted on the probe card and the chuck assembly which supports the test device. The intermediate connector element of a triaxial connector normally is utilized for guarding purposes. However the chuck assembly shown has only a chuck and a shield, with no separate guarding structure to which the intermediate connector element could be connected. Accordingly significant time-consuming alteration of such a station would be required to obtain both a guarded and shielded chuck assembly. The probes on the probe card, on the other hand, are both guarded and shielded; however there is no means of enabling each probe to be moved independently of the others in unison with its guard and shield to accommodate different contact patterns of test devices, thus sacrificing flexibility of the probe station. Also, there is no provision for Kelvin connections on the chuck assembly, which would require more than a single triaxial connector as shown.

Chuck assemblies are available which provide guarding and shielding components. For example, Temptronic Corporation of Newton, Massachusetts markets a thermal chuck assembly atop which is mounted an "add-on" supporting surface for the test device, with a copper guarding layer interposed between the add-on surface and the underlying chuck assembly insulated from each by respective sheets of insulating material. This structure permits a signal line to be soldered to the add-on surface, a guard line to be soldered to the copper guarding layer, and a ground line to be soldered to the underlying chuck assembly which can then serve as a shield. However such wiring requires time-consuming set-up, and particularly so if Kelvin connections are also required. Moreover, the use of sheet insulation to insulate the copper guarding layer from the add-on surface and the underlying chuck assembly fails to provide as low a dielectric constant between the respective elements as is desirable to minimize leakage currents in view of the low level of current to be measured.

Summary of the Invention

The present invention solves the foregoing drawbacks of the prior probe stations by providing a probe station having integrated and ready-to-use guarding, Kelvin connection and shielding systems, both for individually movable probes and for the chuck assembly.

The chuck assembly comprises at least first, second and third chuck assembly elements electrically insulated from one another and positioned at progressively greater distances from the probe-

(s) along the axis of approach between them. At least one detachable electrical connector assembly is provided on the chuck assembly having respective connector elements connected matingly to the first and second chuck assembly elements, respectively, so as to provide a ready-to-use guarding system requiring only the easy detachable connection of a guarded cable to the connector assembly for immediate operability.

Preferably, a second such detachable electrical connector assembly is also provided having its corresponding connector elements connected, in parallel with those of the first connector assembly, to the first and second chuck assembly elements so as to provide a ready-to-use guarded Kelvin connection on the chuck assembly which becomes immediately operable by the easy detachable connection of a second guarded cable to the second connector assembly. Thus one cable serves as a guarded source line and the other serves as a guarded measurement line.

Leakage currents in the chuck assembly are minimized by the fact that the three chuck assembly elements are electrically insulated from one another by distributed patterns of dielectric spacers, rather than continuous dielectric sheets, so that large air gaps are provided between the respective chuck assembly elements to reduce the dielectric constant in the gaps between the elements.

Individually movable probe holders are provided having not only ready-to-use guarded signal line cables and Kelvin connection cables, but also respective shields for the cables of each probe, the shields being movable independently in unison with each probe separately.

The foregoing and other objectives, features, and advantages of the invention will be more readily understood upon consideration of the following detailed description of the invention, taken in conjunction with the accompanying drawings.

Brief Description of the Drawings

FIG. 1 is a partial front view of an exemplary embodiment of a wafer probe station constructed in accordance with the present invention.

FIG. 2 is a top view of the wafer probe station of FIG. 1.

FIG. 2A is a partial top view of the wafer probe station of FIG. 1 with the enclosure door shown partially open.

FIG. 3 is a partially sectional and partially schematic front view of the probe station of FIG. 1.

FIG. 3A is an enlarged sectional view taken along line 3A-3A of FIG. 3.

FIG. 4 is a top view of the sealing assembly where the motorized positioning mechanism extends through the bottom of the enclosure.

FIG. 5A is an enlarged top detail view taken along line 5A-5A of FIG. 1.

FIG. 5B is an enlarged top sectional view taken along line 5B-5B of FIG. 1.

FIG. 6 is a partially schematic top detail view of the chuck assembly, taken along line 6-6 of FIG. 3.

FIG. 7 is a partially sectional front view of the chuck assembly of FIG. 6.

FIG. 8 is a partially sectional side view of a probe holder and probe.

FIG. 9 is a partially sectional bottom view taken along line 9-9 of FIG. 8.

Description of the Preferred Embodiment

General Arrangement of Probe Station

With reference to FIGS. 1, 2 and 3, an exemplary embodiment of the probe station of the present invention comprises a base 10 (shown partially) which supports a platen 12 through a number of jacks 14a, 14b, 14c, 14d which selectively raise and lower the platen vertically relative to the base by a small increment (approximately one-tenth of an inch) for purposes to be described hereafter. Also supported by the base 10 of the probe station is a motorized positioner 16 having a rectangular plunger 18 which supports a movable chuck assembly 20 for supporting a wafer or other test device. The chuck assembly 20 passes freely through a large aperture 22 in the platen 12 which permits the chuck assembly to be moved independently of the platen by the positioner 16 along X, Y and Z axes, i.e. horizontally along two mutually-perpendicular axes X and Y, and vertically along the Z axis. Likewise, the platen 12, when moved vertically by the jacks 14, moves independently of the chuck assembly 20 and the positioner 16.

Mounted atop the platen 12 are multiple individual probe positioners such as 24 (only one of which is shown), each having an extending member 26 to which is mounted a probe holder 28 which in turn supports a respective probe 30 for contacting wafers and other test devices mounted atop the chuck assembly 20. The probe positioner 24 has micrometer adjustments 34, 36 and 38 for adjusting the position of the probe holder 28, and thus the probe 30, along the X, Y and Z axes respectively, relative to the chuck assembly 20. The Z axis is exemplary of what is referred to herein loosely as the "axis of approach" between the probe holder 28 and the chuck assembly 20, although directions of approach which are neither vertical nor linear, along which the probe tip and wafer or other test device are brought into contact with each other, are also intended to be included within the meaning of the term "axis of approach." A further micrometer adjustment 40 adjustably tilts

the probe holder 28 to adjust planarity of the probe with respect to the wafer or other test device supported by the chuck assembly 20. As many as twelve individual probe positioners 24, each supporting a respective probe, may be arranged on the platen 12 around the chuck assembly 20 so as to converge radially toward the chuck assembly similarly to the spokes of a wheel. With such an arrangement, each individual positioner 24 can independently adjust its respective probe in the X, Y and z directions, while the jacks 14 can be actuated to raise or lower the platen 12 and thus all of the positioners 24 and their respective probes in unison.

An environment control enclosure is composed of an upper box portion 42 rigidly attached to the platen 12, and a lower box portion 44 rigidly attached to the base 10. Both portions are made of steel or other suitable electrically conductive material to provide EMI shielding. To accommodate the small vertical movement between the two box portions 42 and 44 when the jacks 14 are actuated to raise or lower the platen 12, an electrically conductive resilient foam gasket 46, preferably composed of silver or carbon-impregnated silicone, is interposed peripherally at their mating juncture at the front of the enclosure and between the lower portion 44 and the platen 12 so that an EMI, substantially hermetic, and light seal are all maintained despite relative vertical movement between the two box portions 42 and 44. Even though the upper box portion 42 is rigidly attached to the platen 12, a similar gasket 47 is preferably interposed between the portion 42 and the top of the platen to maximize sealing.

With reference to FIGS. 5A and 5B, the top of the upper box portion 42 comprises an octagonal steel box 48 having eight side panels such as 49a and 49b through which the extending members 26 of the respective probe positioners 24 can penetrate movably. Each panel comprises a hollow housing in which a respective sheet 50 of resilient foam, which may be similar to the above-identified gasket material, is placed. Slits such as 52 are partially cut vertically in the foam in alignment with slots 54 formed in the inner and outer surfaces of each panel housing, through which a respective extending member 26 of a respective probe positioner 24 can pass movably. The slitted foam permits X, Y and Z movement of the extending members 26 of each probe positioner, while maintaining the EMI, substantially hermetic, and light seal provided by the enclosure. In four of the panels, to enable a greater range of X and Y movement, the foam sheet 50 is sandwiched between a pair of steel plates 55 having slots 54 therein, such plates being slidable transversely within the panel housing through a range of movement encompassed by

larger slots 56 in the inner and outer surfaces of the panel housing.

Atop the octagonal box 48, a circular viewing aperture 58 is provided, having a recessed circular transparent sealing window 60 therein. A bracket 62 holds an apertured sliding shutter 64 to selectively permit or prevent the passage of light through the window. A stereoscope (not shown) connected to a CRT monitor can be placed above the window to provide a magnified display of the wafer or other test device and the probe tip for proper probe placement during set-up or operation. Alternatively, the window 60 can be removed and a microscope lens (not shown) surrounded by a foam gasket can be inserted through the viewing aperture 58 with the foam providing EMI, hermetic and light sealing.

The upper box portion 42 of the environment control enclosure also includes a hinged steel door 68 which pivots outwardly about the pivot axis of a hinge 70 as shown in FIG. 2A. The hinge biases the door downwardly toward the top of the upper box portion 42 so that it forms a tight, overlapping, sliding peripheral seal 68a with the top of the upper box portion. When the door is open, and the chuck assembly 20 is moved by the positioner 16 beneath the door opening as shown in FIG. 2A, the chuck assembly is accessible for loading and unloading.

With reference to FIGS. 3 and 4, the sealing integrity of the enclosure is likewise maintained throughout positioning movements by the motorized positioner 16 due to the provision of a series of four sealing plates 72, 74, 76 and 78 stacked slidably atop one another. The sizes of the plates progress increasingly from the top to the bottom one, as do the respective sizes of the central apertures 72a, 74a, 76a and 78a formed in the respective plates 72, 74, 76 and 78, and the aperture 79a formed in the bottom 44a of the lower box portion 44. The central aperture 72a in the top plate 72 mates closely around the bearing housing 18a of the vertically-movable plunger 18. The next plate in the downward progression, plate 74, has an upwardly-projecting peripheral margin 74b which limits the extent to which the plate 72 can slide across the top of the plate 74. The central aperture 74a in the plate 74 is of a size to permit the positioner 16 to move the plunger 18 and its bearing housing 18a transversely along the X and Y axes until the edge of the top plate 72 abuts against the margin 74b of the plate 74. The size of the aperture 74a is, however, too small to be uncovered by the top plate 72 when such abutment occurs, and therefore a seal is maintained between the plates 72 and 74 regardless of the movement of the plunger 18 and its bearing housing along the X and Y axes. Further movement of the plunger 18

and bearing housing in the direction of abutment of the plate 72 with the margin 74b results in the sliding of the plate 74 toward the peripheral margin 76b of the next underlying plate 76. Again, the central aperture 76a in the plate 76 is large enough to permit abutment of the plate 74 with the margin 76b, but small enough to prevent the plate 74 from uncovering the aperture 76a, thereby likewise maintaining the seal between the plates 74 and 76. Still further movement of the plunger 18 and bearing housing in the same direction causes similar sliding of the plates 76 and 78 relative to their underlying plates into abutment with the margin 78b and the side of the box portion 44, respectively, without the apertures 78a and 79a becoming uncovered. This combination of sliding plates and central apertures of progressively increasing size permits a full range of movement of the plunger 18 along the X and Y axes by the positioner 16, while maintaining the enclosure in a sealed condition despite such positioning movement. The EMI sealing provided by this structure is effective even with respect to the electric motors of the positioner 16, since they are located below the sliding plates.

Chuck Assembly

With particular reference to FIGS. 3, 6 and 7, the chuck assembly 20 is of a unique modular construction usable either with or without an environment control enclosure. The plunger 18 supports an adjustment plate 79 which in turn supports first, second and third chuck assembly elements 80, 81 and 83, respectively, positioned at progressively greater distances from the probe(s) along the axis of approach. Element 83* is a conductive rectangular stage or shield 83 which detachably mounts conductive elements 80 and 81 of circular shape. The element 80 has a planar upwardly-facing wafer-supporting surface 82 having an array of vertical apertures 84 therein. These apertures communicate with respective chambers separated by O-rings 88, the chambers in turn being connected separately to different vacuum lines 90a, 90b, 90c (FIG. 6) communicating through separately-controlled vacuum valves (not shown) with a source of vacuum. The respective vacuum lines selectively connect the respective chambers and their apertures to the source of vacuum to hold the wafer, or alternatively isolate the apertures from the source of vacuum to release the wafer, in a conventional manner. The separate operability of the respective chambers and their corresponding apertures enables the chuck to hold wafers of different diameters.

In addition to the circular elements 80 and 81, auxiliary chucks such as 92 and 94 are detachably mounted on the corners of the element 83 by

screws (not shown) independently of the elements 80 and 81 for the purpose of supporting contact substrates and calibration substrates while a wafer or other test device is simultaneously supported by the element 80. Each auxiliary chuck 92, 94 has its own separate upwardly-facing planar surface 100, 102 respectively, in parallel relationship to the surface 82 of the element 80. Vacuum apertures 104 protrude through the surfaces 100 and 102 from communication with respective chambers within the body of each auxiliary chuck. Each of these chambers in turn communicates through a separate vacuum line and a separate independently-actuated vacuum valve (not shown) with a source of vacuum, each such valve selectively connecting or isolating the respective sets of apertures 104 with respect to the source of vacuum independently of the operation of the apertures 84 of the element 80, so as to selectively hold or release a contact substrate or calibration substrate located on the respective surfaces 100 and 102 independently of the wafer or other test device. An optional metal shield 106 may protrude upwardly from the edges of the element 83 to surround the other elements 80, 81 and the auxiliary chucks 92, 94.

All of the chuck assembly elements 80, 81 and 83, as well as the additional chuck assembly element 79, are electrically insulated from one another even though they are constructed of electrically conductive metal and interconnected detachably by metallic screws such as 96. With reference to FIGS. 3 and 3A, the electrical insulation results from the fact that, in addition to the resilient dielectric O-rings 88, dielectric spacers 85 and dielectric washers 86 are provided. These, coupled with the fact that the screws 96 pass through oversized apertures in the lower one of the two elements which each screw joins together thereby preventing electrical contact between the shank of the screw and the lower element, provide the desired insulation. As is apparent in FIG. 3, the dielectric spacers 85 extend over only minor portions of the opposing surface areas of the interconnected chuck assembly elements, thereby leaving air gaps between the opposing surfaces over major portions of their respective areas. Such air gaps minimize the dielectric constant in the spaces between the respective chuck assembly elements, thereby correspondingly minimizing the capacitance between them and the ability for electrical current to leak from one element to another. Preferably the spacers and washers 85 and 86, respectively, are constructed of a material having the lowest possible dielectric constant consistent with high dimensional stability and high volume resistivity. A suitable material for the spacers and washers is glass epoxy, or acetal homopolymer marketed under the trademark Delrin by E.I. DuPont.

With reference to FIGS. 6 and 7, the chuck assembly 20 also includes a pair of detachable electrical connector assemblies designated generally as 108 and 110, each having at least two conductive connector elements 108a, 108b and 110a, 110b, respectively, electrically insulated from each other, with the connector elements 108b and 110b preferably coaxially surrounding the connector elements 108a and 110a as guards therefor. If desired, the connector assemblies 108 and 110 can be triaxial in configuration so as to include respective outer shields 108c, 110c surrounding the respective connector elements 108b and 110b, as shown in FIG. 7. The outer shields 108c and 110c may, if desired, be connected electrically through a shielding box 112 and a connector supporting bracket 113 to the chuck assembly element 83, although such electrical connection is optional particularly in view of the surrounding EMI shielding enclosure 42, 44. In any case, the respective connector elements 108a and 110a are electrically connected in parallel to a connector plate 114 matingly and detachably connected along a curved contact surface 114a by screws 114b and 114c to the curved edge of the chuck assembly element 80. Conversely, the connector elements 108b and 110b are connected in parallel to a connector plate 116 similarly matingly connected detachably to element 81. The connector elements pass freely through a rectangular opening 112a in the box 112, being electrically insulated from the box 112 and therefore from the element 83, as well as being electrically insulated from each other. Set screws such as 118 detachably fasten the connector elements to the respective connector plates 114 and 116.

Either coaxial or, as shown, triaxial cables 118 and 120 form portions of the respective detachable electrical connector assemblies 108 and 110, as do their respective triaxial detachable connectors 122 and 124 which penetrate a wall of the lower portion 44 of the environment control enclosure so that the outer shields of the triaxial connectors 122, 124 are electrically connected to the enclosure. Further triaxial cables 122a, 124a are detachably connectable to the connectors 122 and 124 from suitable test equipment such as a Hewlett-Packard 4142B modular DC source/monitor or a Hewlett-Packard 4284A precision LCR meter, depending upon the test application. If the cables 118 and 120 are merely coaxial cables or other types of cables having only two conductors, one conductor interconnects the inner (signal) connector element of a respective connector 122 or 124 with a respective connector element 108a or 110a, while the other conductor connects the intermediate (guard) connector element of a respective connector 122 or 124 with a respective connector element 108b, 110b.

In any case, the detachable connector assemblies 108, 110, due to their interconnections with the two connector plates 114, 116, provide immediately ready-to-use signal and guard connections to the chuck assembly elements 80 and 81, respectively, as well as ready-to-use guarded Kelvin connections thereto. For applications requiring only guarding of the chuck assembly, as for example the measurement of low-current leakage from a test device through the element 80, it is necessary only that the operator connect a single guarded cable 122a from a test instrument such as a Hewlett-Packard 4142B modular DC source/monitor to the detachable connector 122 so that a signal line is provided to the chuck assembly element 80 through the connector element 108a and connector plate 114, and a guard line is provided to the element 81 through the connector element 108b and connector plate 116. Alternatively, if a Kelvin connection to the chuck assembly is desired for low-voltage measurements, such as those needed for measurements of low capacitance, the operator need merely attach a pair of cables 122a and 124a to the respective connectors 122, 124 from a suitable test instrument such as a Hewlett-Packard 4284A precision LCR meter, thereby providing both source and measurement lines to the element 80 through the connector elements 108a and 110a and connector plate 114, and guarding lines to the element 81 through the connector elements 108b and 110b and connector plate 116.

Probe Assembly

With reference to FIGS. 5B, 8 and 9, respective individually movable probes 30 comprising pairs of probe elements 30a are supported by respective probe holders 28 which in turn are supported by respective extending portions 26 of different probe positioners such as 24. Atop each probe positioner 24 is a shield box 126 having a pair of triaxial connectors 128, 130 mounted thereon with respective triaxial cables 132 entering each triaxial connector from a suitable test instrument as mentioned previously. Each triaxial connector includes a respective inner connector element 128a, 130a, an intermediate connector element 128b, 130b, and an outer connector element 128c, 130c in concentric arrangement. Each outer connector element 128c, 130c terminates by connection with the shield box 126. Conversely, the inner connector elements 128a, 130a, and the intermediate connector elements 128b, 130b, are connected respectively to the inner and outer conductors of a pair of coaxial cables 134, 136 which therefore are guarded cables. Each cable 134, 136 terminates through a respective coaxial connector 138, 140 with a respective probe element 30a having a center con-

ductor 142 surrounded by a guard 144. In order to provide adequate shielding for the coaxial cables 134, 136, especially in the region outside of the octagonal box 48, an electrically-conductive shield tube 146 is provided around the cables 134, 136 and electrically connected through the shield box 126 with the outer connector element 128c, 130c of the respective triaxial connectors 128, 130. The shield tube 146 passes through the same slit in the foam 50 as does the underlying extending member 26 of the probe positioner 24. Thus each individually movable probe 30 has not only its own separate individually movable probe holder 28 but also its own individually movable shield 146 for its guarded coaxial cables, which shield is movable in unison with the probe holder independently of the movement of any other probe holder by any other positioning mechanism 24. This feature is particularly advantageous because such individually movable probes are normally not equipped for both shielded and guarded connections, which deficiency is solved by the described structure. Accordingly, the probes 30 are capable of being used with the same guarding and Kelvin connection techniques in a ready-to-use manner as is the chuck assembly 20, consistently with full shielding despite the individual positioning capability of each probe 30.

The terms and expressions which have been employed in the foregoing specification are used therein as terms of description and not of limitation, and there is no intention, in the use of such terms and expressions, of excluding equivalents of the features shown and described or portions thereof, it being recognized that the scope of the invention is defined and limited only by the claims which follow.

Claims

1. A probe station comprising:

- (a) a chuck assembly for holding a test device;
- (b) a holder for an electrical probe for contacting the test device;
- (c) a positioning mechanism for selectively moving at least one of said chuck assembly and said holder toward or away from the other along an axis of approach;
- (d) said chuck assembly comprising at least separate first, second and third chuck assembly elements electrically insulated from one another and positioned at progressively greater distances from said holder along said axis of approach, characterized in that said chuck assembly further includes at least one detachable electrical connector assembly for detachably receiving a cable

from a test instrument, said connector assembly having at least two conductive connector elements electrically insulated from one another, each of said connector elements being electrically connected matingly to a different respective one of said first and second chuck assembly elements and neither being electrically connected to said third chuck assembly element.

- 2. The probe station of claim 1 wherein said chuck assembly includes a further said detachable electrical connector assembly having at least two further conductive connector elements each electrically connected to a different respective one of said first and second chuck assembly elements in parallel with the connector elements of said one detachable electrical connector assembly.
- 3. The probe station of claim 1 wherein each of said connector elements is detachably matingly connected to a different respective one of said first and second chuck assembly elements.
- 4. The probe station of claim 1 wherein a first one of said connector elements is surrounded by a second one of said connector elements, the first connector element being electrically connected to said first chuck assembly element, and the second connector element being electrically connected to said second chuck assembly element.
- 5. The probe station of claim 4 wherein said chuck assembly includes a further said detachable electrical connector assembly having further ones of said first and second connector elements electrically connected to said first and second chuck assembly elements in parallel with said first and second connector elements.
- 6. The probe station of claim 1 wherein each of said chuck assembly elements further includes at least one surface area facing toward a surface area of another one of said chuck assembly elements, said chuck assembly further including dielectric spacers located between the respective surface areas of the respective chuck assembly elements, said spacers extending over only portions of said surface areas so as to leave air gaps between other portions of said surface areas.
- 7. The probe station of claim 6, further including threaded fasteners extending through said

spacers between the respective surface areas of said chuck assembly elements, and respective insulators for electrically insulating said fasteners from at least one of said surface areas.

5

8. The probe station of claim 1 wherein said positioning mechanism includes means for selectively moving said holder toward or away from said chuck assembly along an axis of approach and for selectively moving said holder relative to said chuck assembly along other axes perpendicular to said axis of approach, further including at least one electrical connector associated with said holder and having first, second, and third connector elements electrically insulated from each other, an electrical cable, having first and second conductors electrically connected separately to said first and second connector elements, respectively, for interconnecting said first and second connector elements with said electrical probe, and an electrically conductive shield surrounding said electrical cable for shielding said cable against electromagnetic interference, said shield being electrically connected to said third connector element and being movable by said positioning mechanism in unison with said holder along said axis of approach and along said other axes.
9. The probe station of claim 8 wherein said electrical connector is of a triaxial configuration having substantially concentric inner, intermediate and outer connector elements which comprise said first, second and third connector elements respectively, and wherein said electrical cable is a coaxial cable having substantially concentric inner and outer conductors which comprise said first and second conductors respectively.
10. The probe station of claim 8 including a further said electrical connector having further first, second and third connector elements, and a further electrical cable having first and second conductors electrically connected separately to said further first and second connector elements, said shield also surrounding said further electrical cable.
11. The probe station of claim 8 including a further positioning mechanism for selectively moving a further holder for an electrical probe with respect to said chuck assembly, said shield being movable independently of any movement by said further positioning mechanism.

10

15

20

25

30


35


40


45

50

55

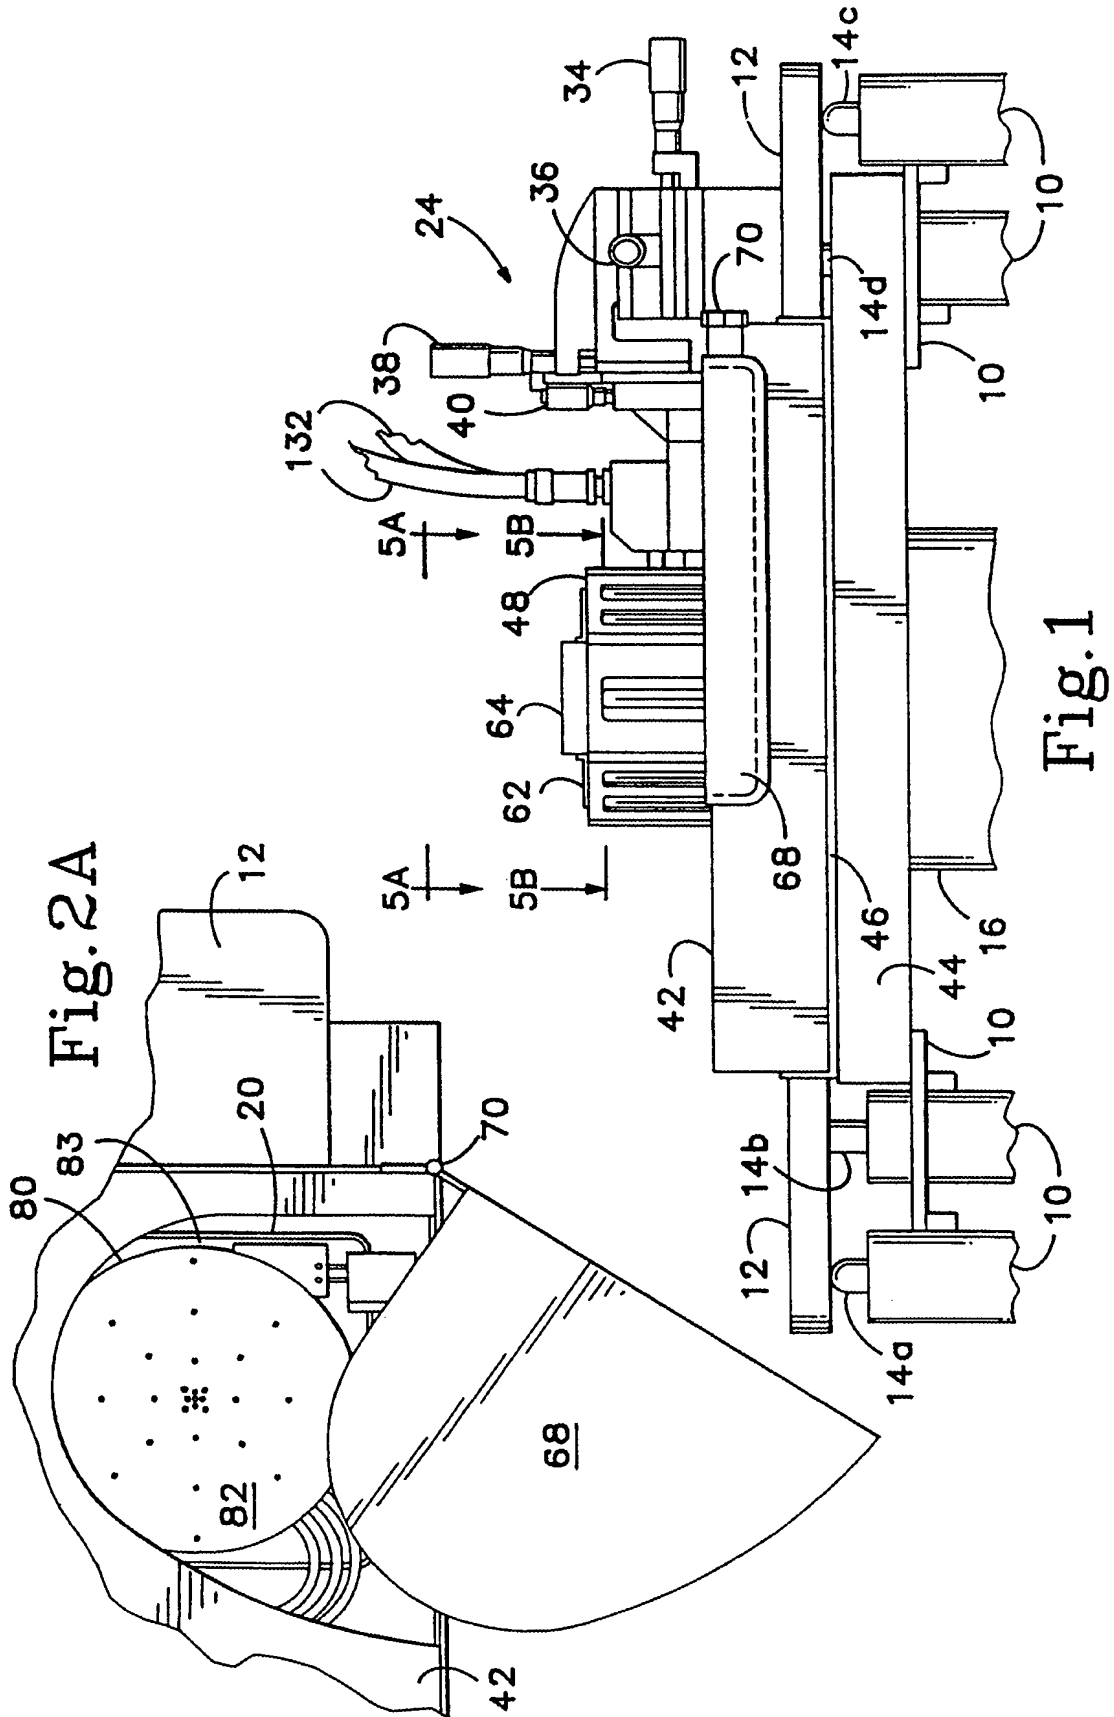

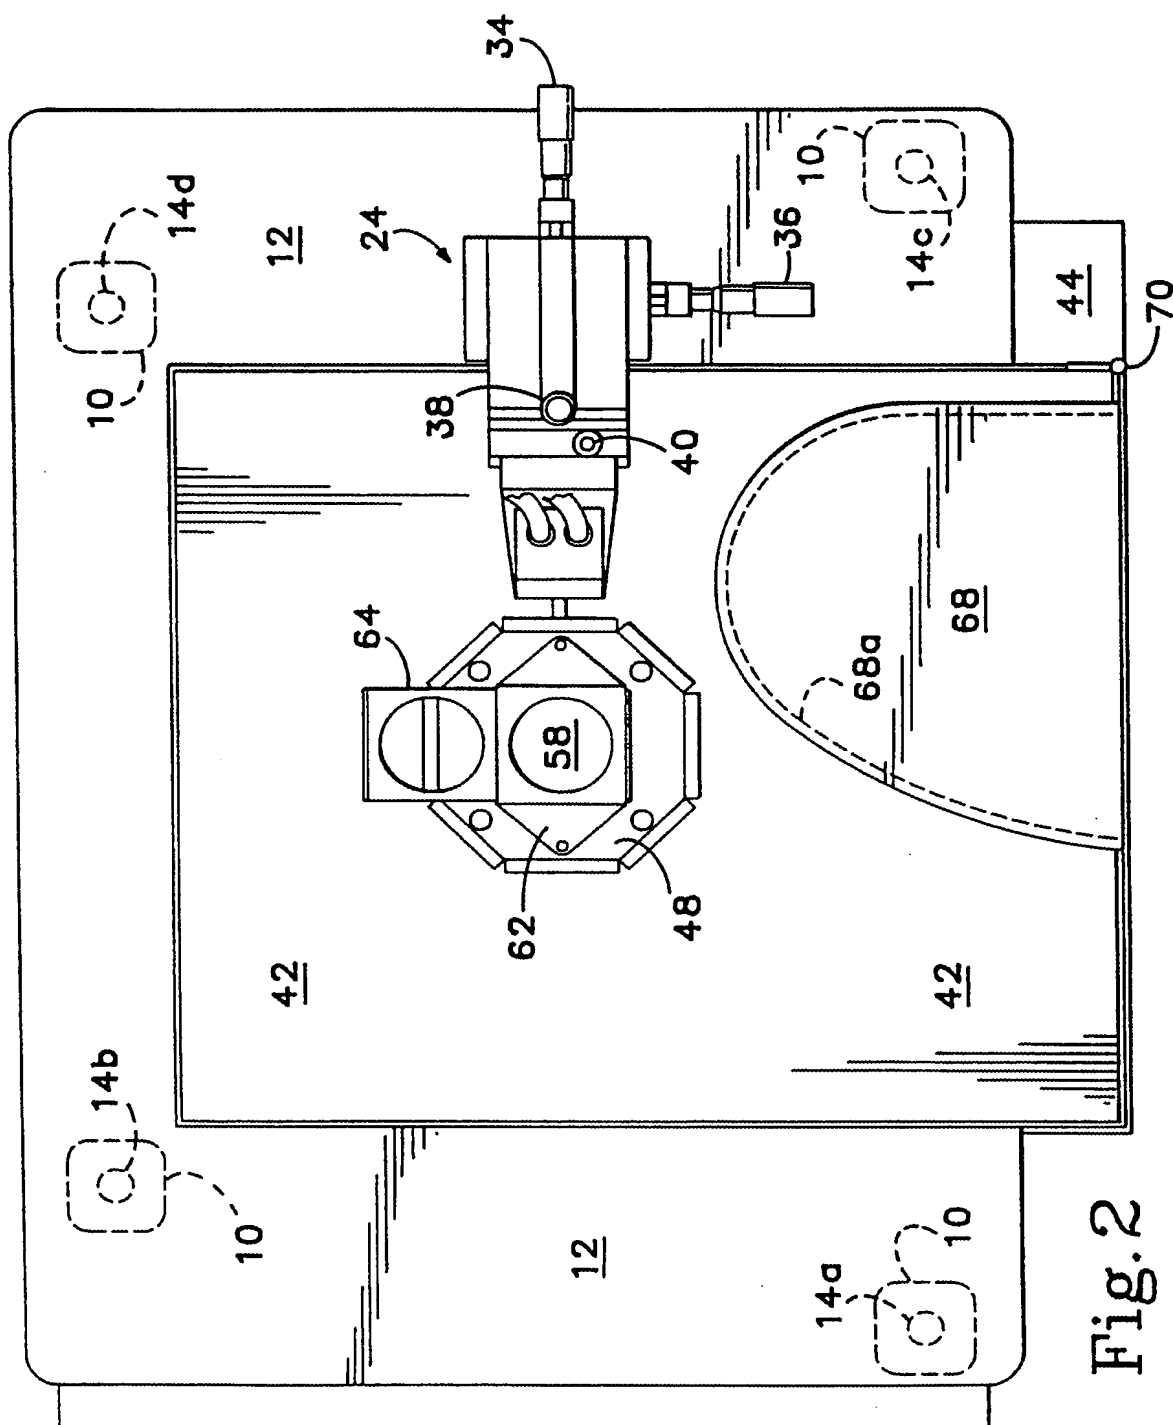

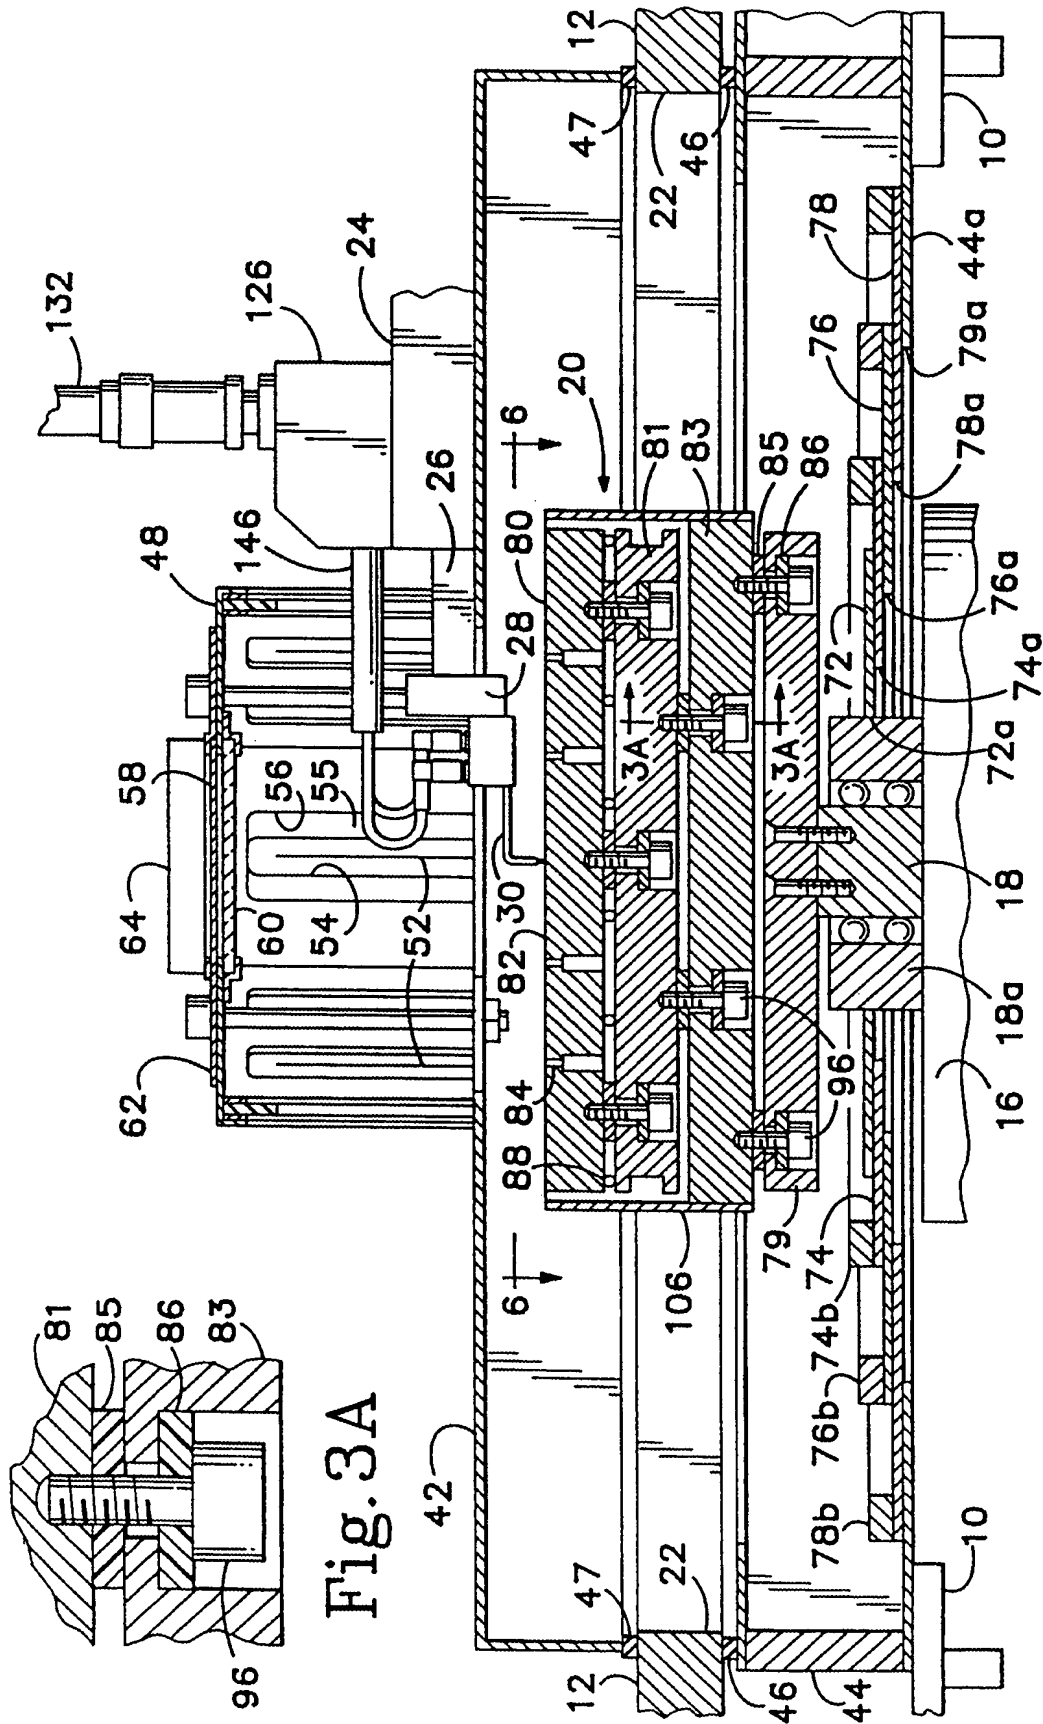

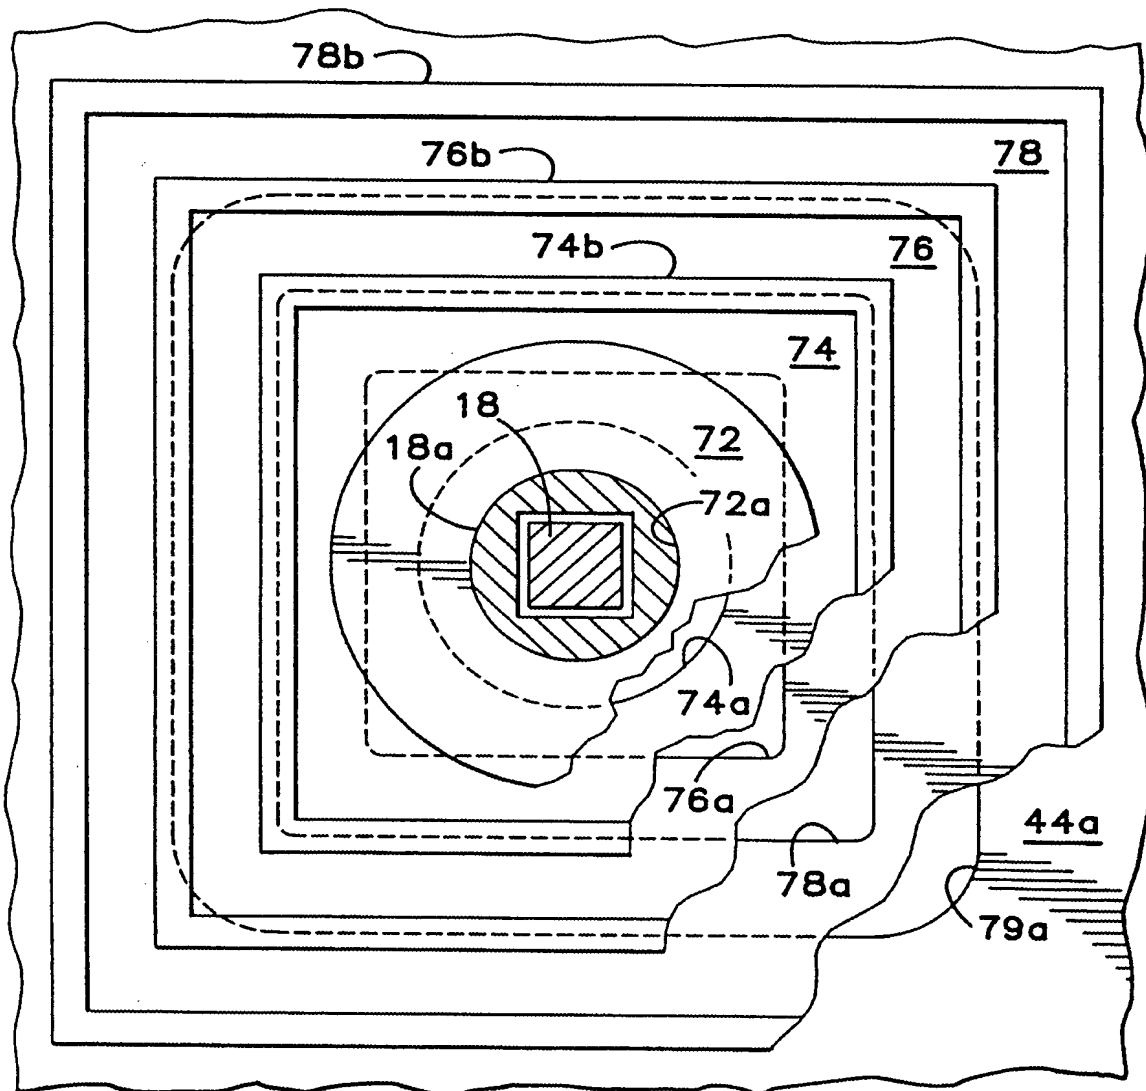
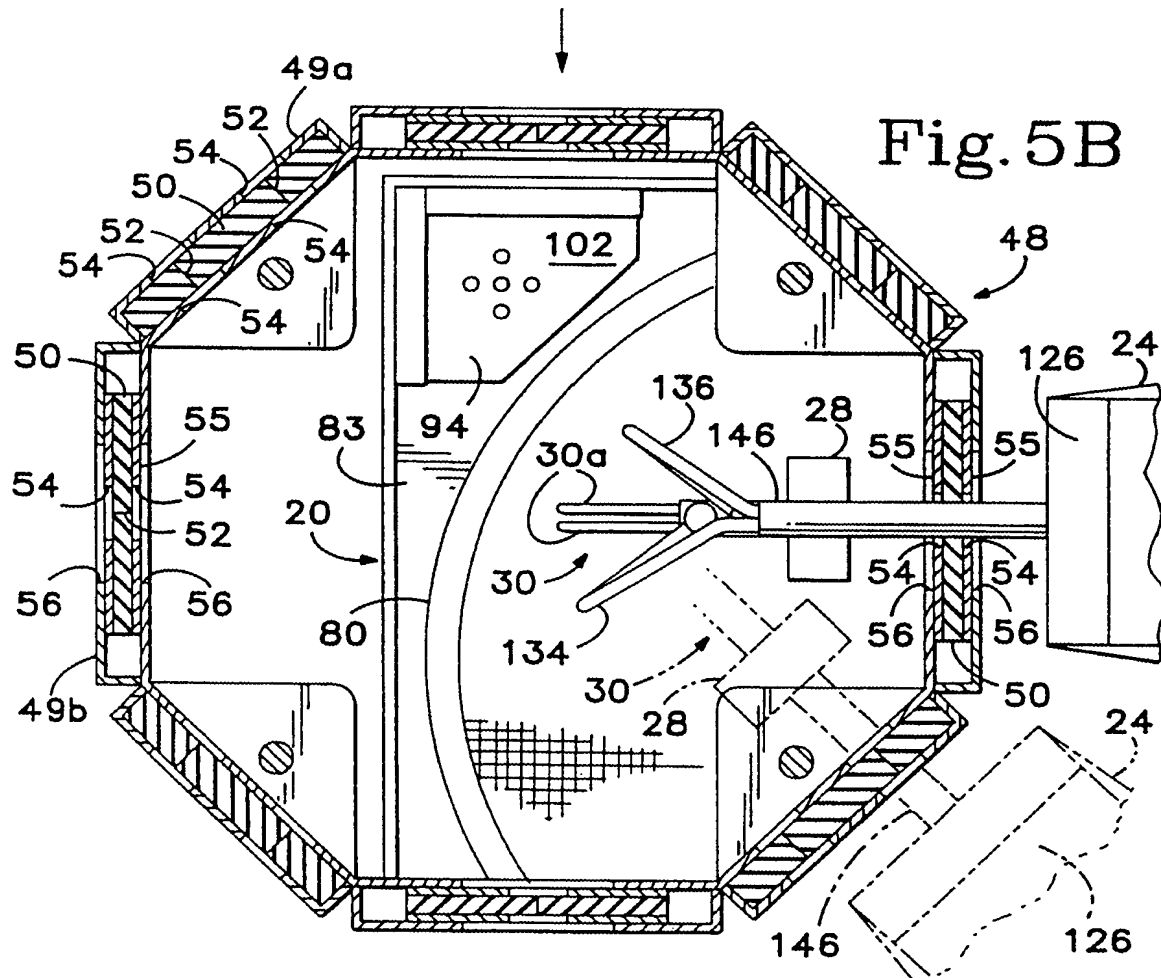
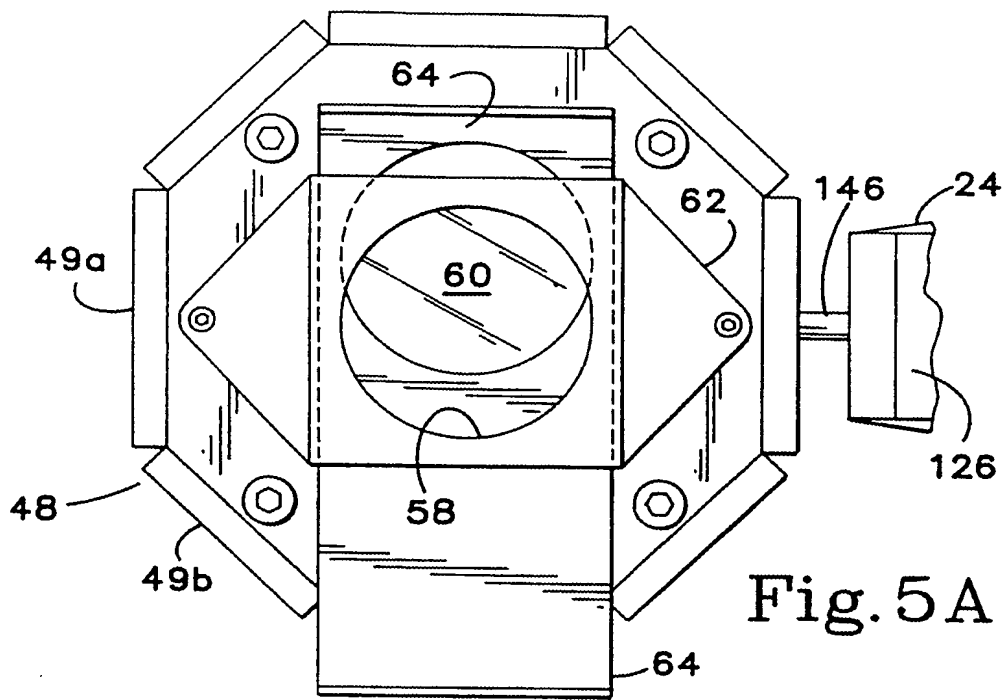


Fig. 4



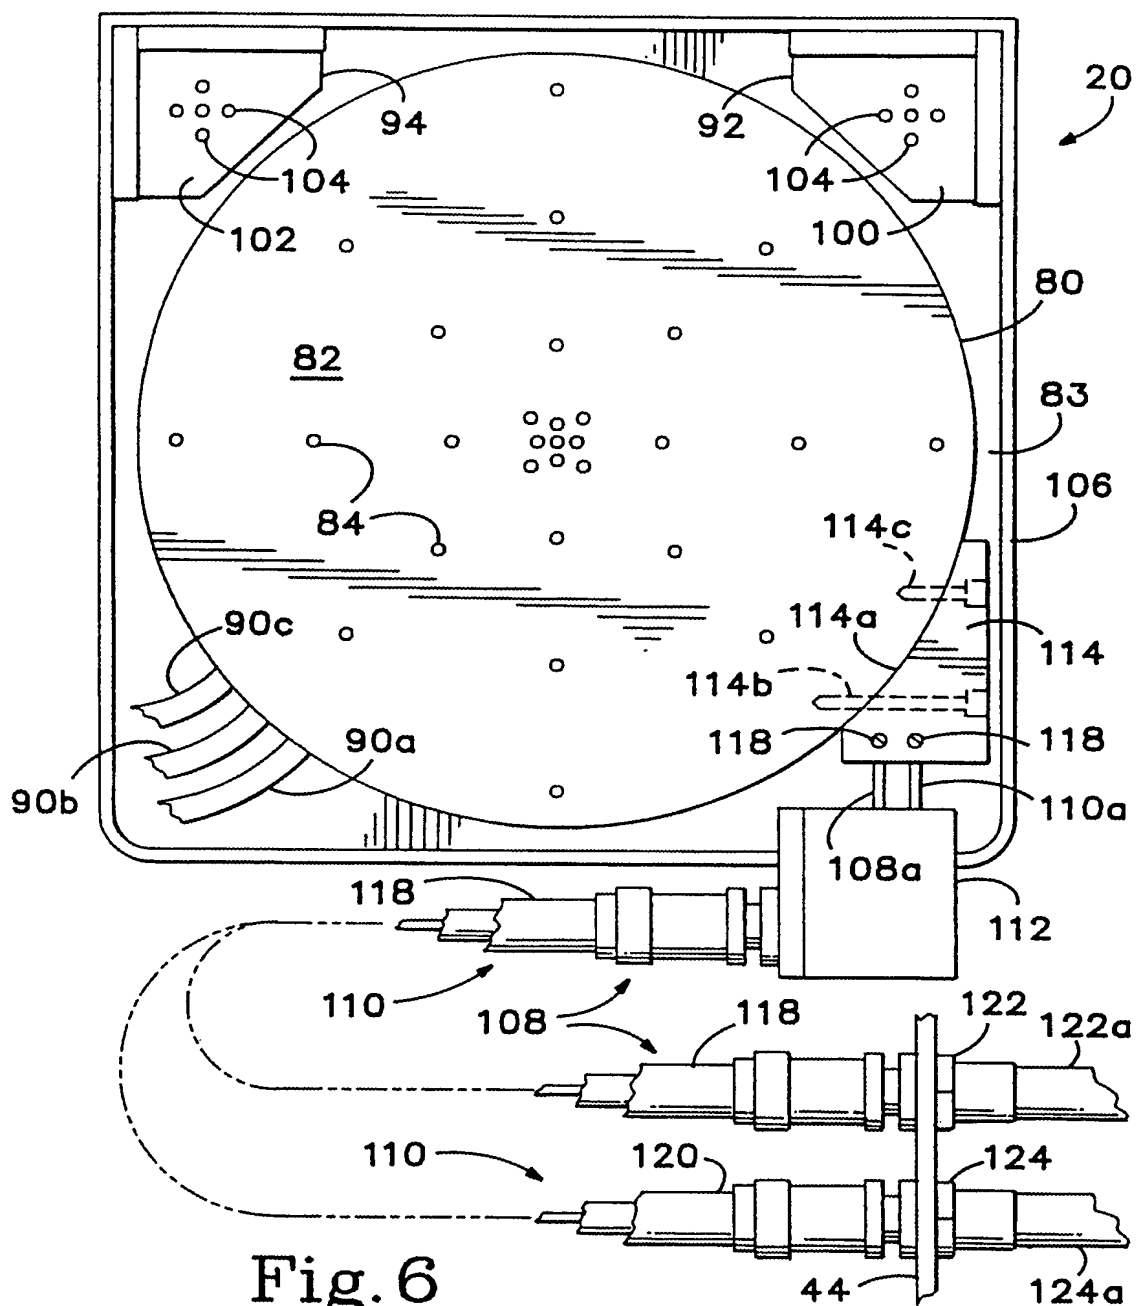


Fig. 6

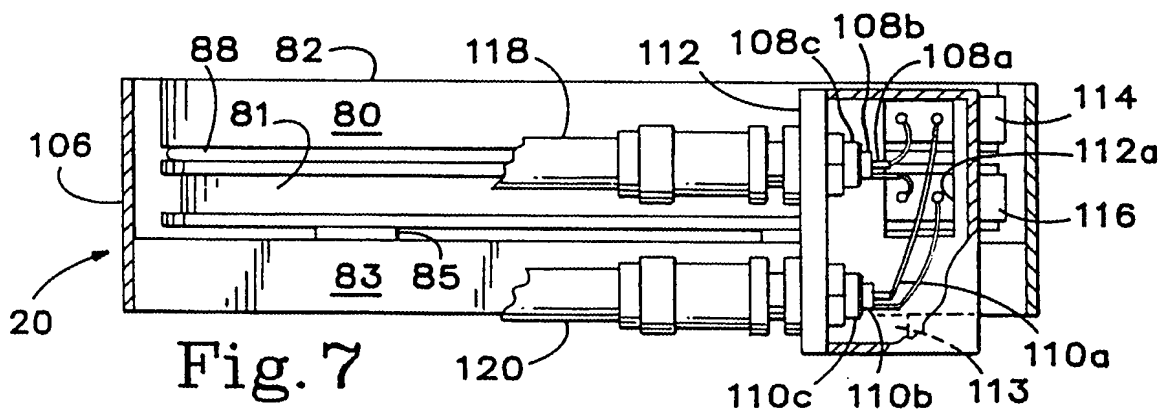


Fig. 7


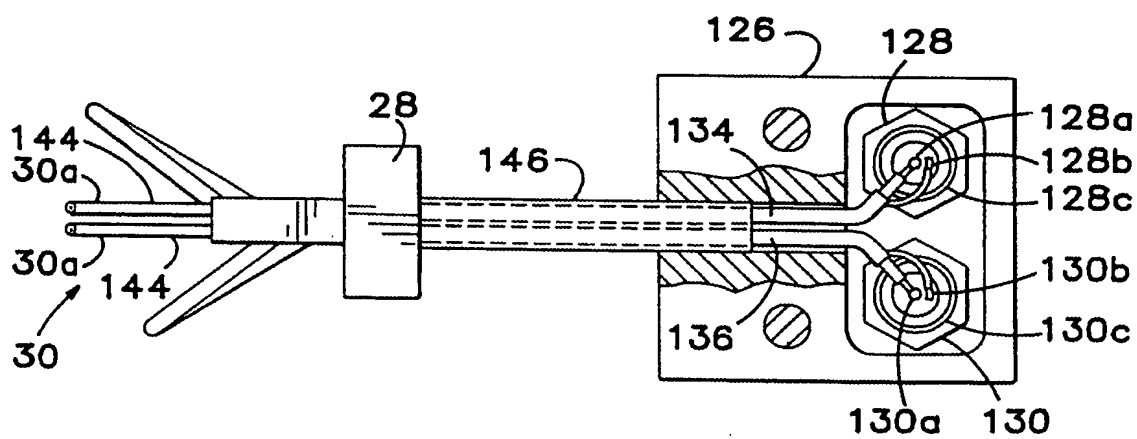


Fig. 9

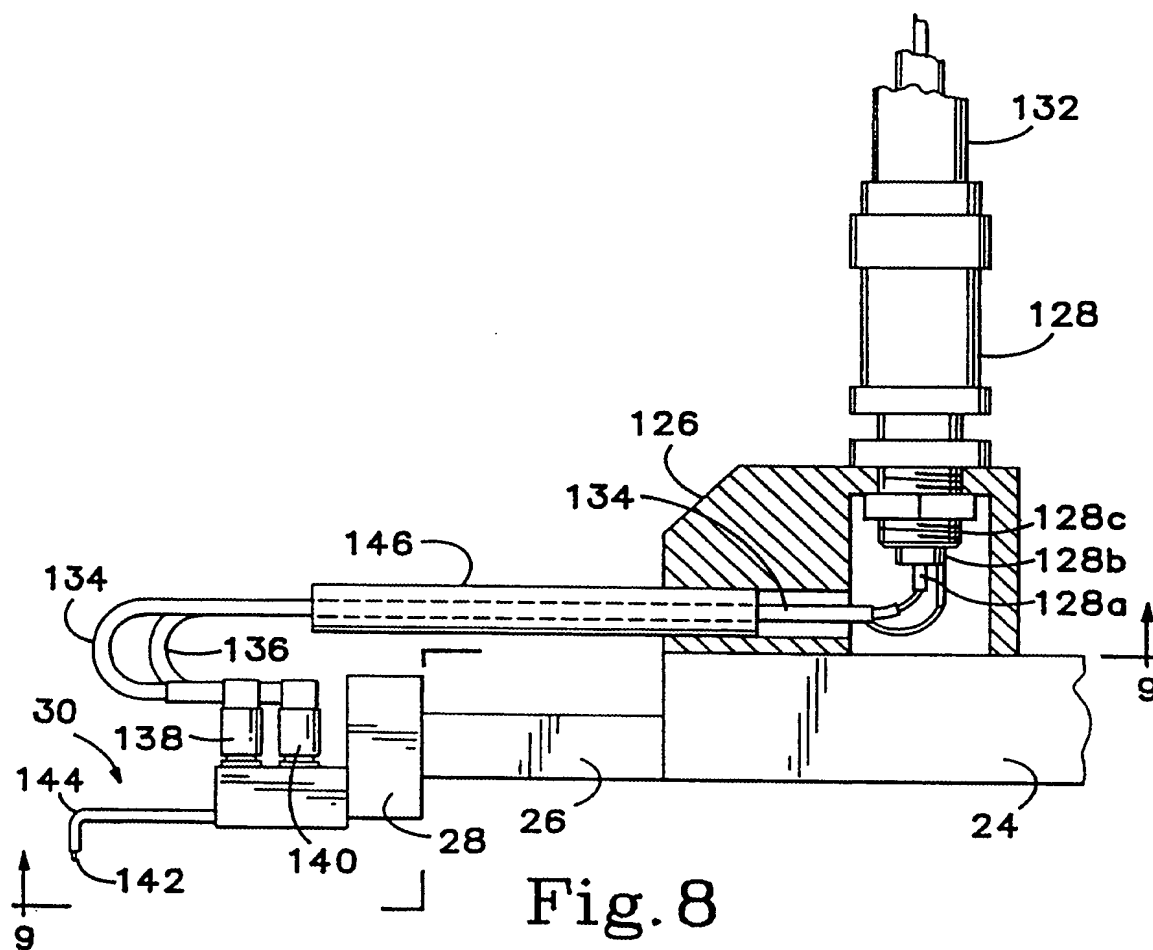

European Patent
Office

EUROPEAN SEARCH REPORT

Application Number

EP 93 30 3936

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int. Cl.5)
A	EP-A-0 201 205 (PROMETRIX) * column 15, line 50 - column 16, line 29 * * column 23, line 6 - column 24, line 46; claim 1; figures 11,22-24 *	1,8,11	H01L21/00
A	US-A-4 056 777 (ROCH) * column 4, line 53 - column 7, line 54; claim 1; figures 1-4 *	1,8	
D,A	EVALUATION ENGINEERING November 1990, NOKOMIS US pages 150 - 153 WILLIAM KNAUER 'FIXTURING FOR LOW CURRENT/LOW VOLTAGE PARAMETRIC TESTING' * page 151, middle column, paragraph 2 - page 152, middle column, last paragraph; figure 2 *	1,2,4,5, 8-10	
D,A	IEEE TRANSACTIONS ON INSTRUMENTATION AND MEASUREMENT vol. 38, no. 6, December 1989, NEW YORK US pages 1088 - 1093 , XP000095937 YOUSOUKE YAMAMOTO 'A COMPACT SELF SHIELDING PROBER FOR ACCURATE MEASURE- MENT OF ON WAFER ELECTRON DEVICE.' * page 1088, right column, paragraph II.A - page 1089, right column, paragraph II.C; figures 1,3,4 *	1	TECHNICAL FIELDS SEARCHED (Int. Cl.5) H01L G01R
The present search report has been drawn up for all claims			
Place of search THE HAGUE		Date of completion of the search 15 SEPTEMBER 1993	Examiner RIEUTORT A.S.
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons ----- Δ : member of the same patent family, corresponding document	

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☒ FADED TEXT OR DRAWING
- ☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☐ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☒ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.